


## Hepatitis B Virus (HBV) Assay diagram for Look-Back Procedure

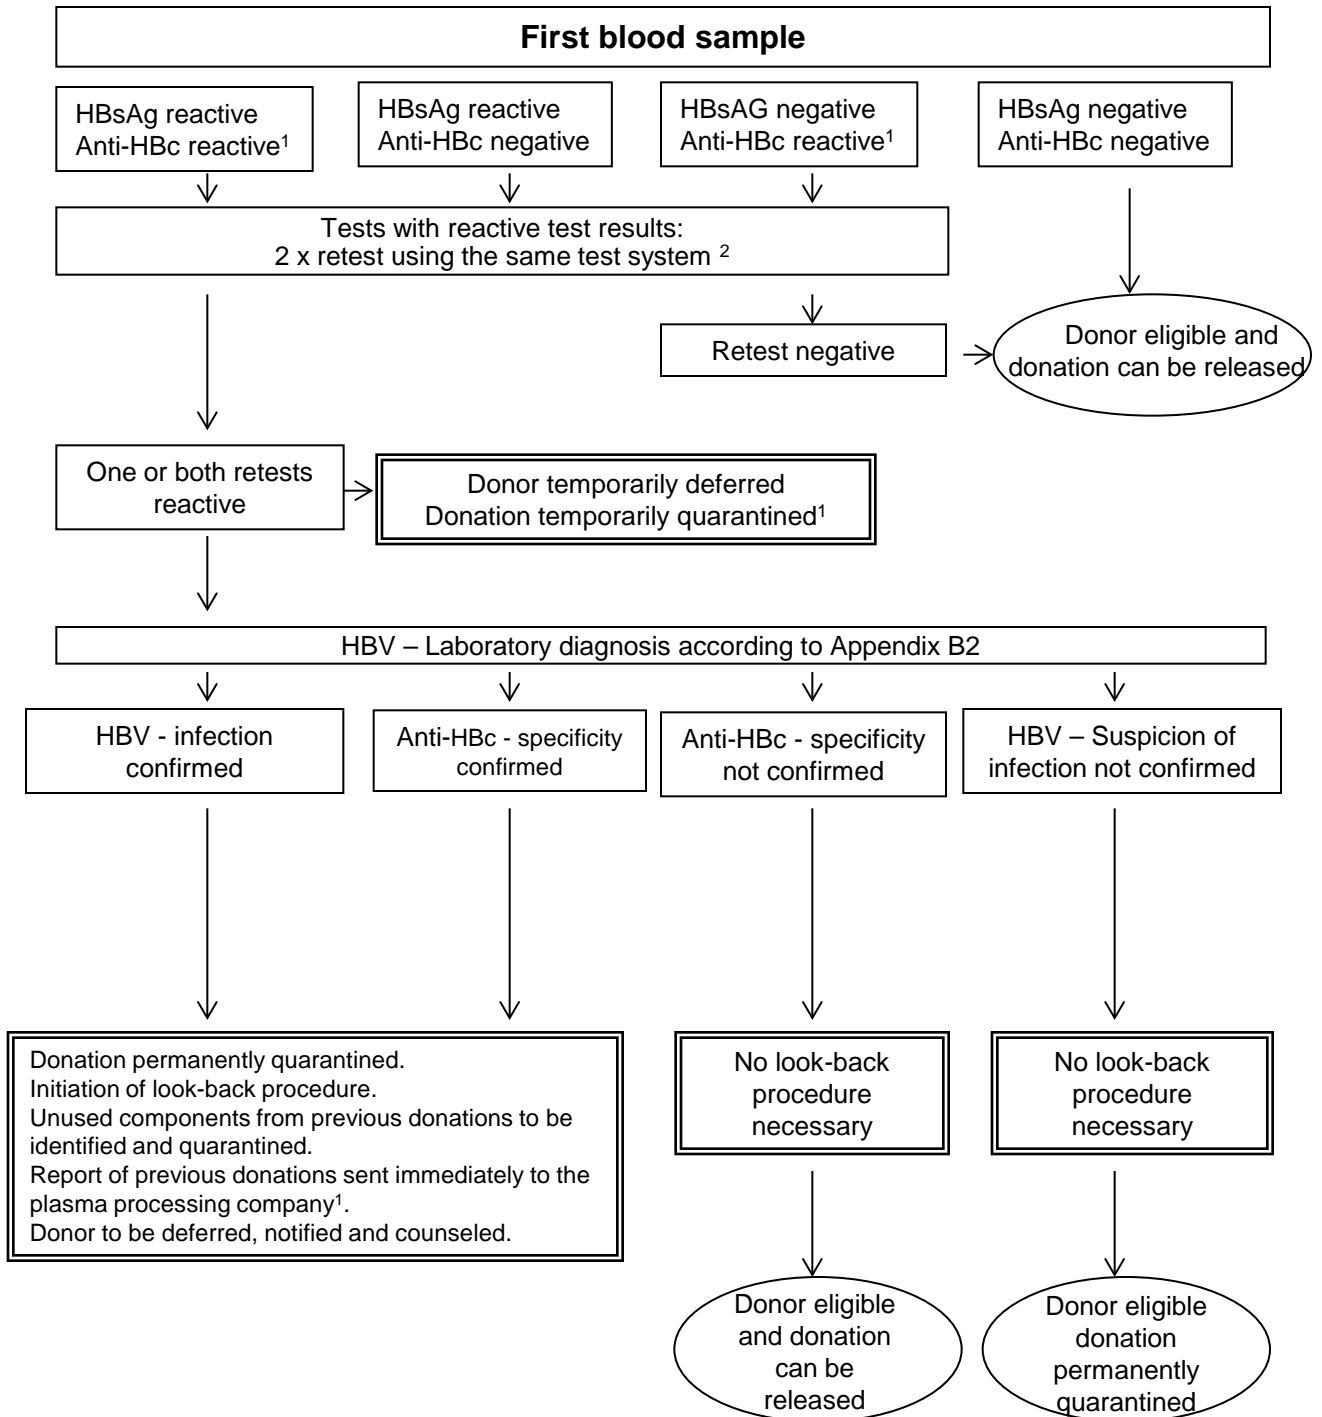

1. Reactive Anti-HBc results have no bearing on use of plasma for fractionation.
2. In cases with detectable HBV-DNA the test result is considered to be confirmed positive regardless of results obtained from tests performed according to Appendix B2.